

# **Silicon Oxynitride Waveguides as Evanescent Field Based **Fluorescent** Biosensors**

F.J. Aparicio,<sup>1\*</sup> E. Froner,<sup>1</sup> E. Rigo<sup>1</sup>, D. Gandolfi,<sup>1</sup> M. Scarpa,<sup>1</sup> B. Han,<sup>1,2</sup> M.

Ghulinyan,<sup>2</sup> G. Pucker,<sup>2</sup> and L. Pavesi<sup>1</sup>

<sup>1</sup>Nanoscience Laboratory, Department of Physics, University of Trento, via Sommarive  
14, 38123 Povo, Italy

<sup>2</sup>Center for Materials and Microsystems, Fondazione Bruno Kessler, Povo – Trento  
38123, Italy

\*Corresponding author: [fjaparicio@icmse.csic.es](mailto:fjaparicio@icmse.csic.es)

**ABSTRACT:** Channel waveguide based evanescent-field optical sensors were developed to make a fully integrated chip biosensor. The optical system senses fluorescent analytes immobilized within a micrometric sized bio-reactor well realized within an optical waveguide. The main novelty of this work is related to the fact that, within the bioreactor well, the excitation of the fluorescent signal is achieved by means of the evanescent field propagating through a silicon oxynitride waveguide. The immobilization of the emitting molecules has been realized by functionalization of the waveguide surface by a wet chemical method. These photonic biosensors are successfully applied to detect low surface concentration ( $10^{-11}$  mol/cm<sup>2</sup>) of a green emitting organic dye. This approach could permit the selective detection of a wide range of chemical and biological species in complex matrices and can be exploited to set-up array-based screening devices. In this regards, the preferential excitation of the dye molecules in the close vicinity of the exposed waveguide core is also analyzed.

## Introduction

Compact and portable chip-biosensor devices able to perform laboratory operations at the end-user premise are very attractive in a wide range of fields such as: medicine, biology, defense, and food industry [1-3]. The most diffused approach for such lab-on-a-chip biosensors is based on disposable optical micro-transducers functionalized with a biological layer (e.g. antibodies, enzymes, DNA, aptamers, and scaffolds [4,5]) for the selective immobilization of the target analyte [1,6,7]. Beside the high sensitivity, reliability, immunity to electromagnetic interference, and fast response of the optical techniques, one of the main properties of these approaches is the high selectivity of the bio-recognition event [4]. A higher degree of selectivity is reached in case of the

fluorescent based "sandwich" approach. This is a two-step recognition method whereby the target biomolecules are selectively marked with a fluorescent tag in addition to the selective immobilization on the bio-receptor layer [1]. This approach eliminates the need to purify the analyte from complicated mixtures before the measurement, simplifies the assay, and increases the sensitivity by the use of fluorescent markers. To fully exploit this selectivity, it is needed to confine the interrogation volume (i.e. the interaction volume of the optical probe) to the biorecognition layer where the target biomolecules are immobilized. In this way only the analytes selectively bound to the structure are labelled and detected, while the excess of fluorescent markers floating in the sample solution does not contribute to the signal. This is successfully accomplished by making use of the evanescent field of the optical mode propagating through a waveguide structure. When a light wave is coupled into a waveguide, the associated electromagnetic field is not completely confined to the waveguide core; but it exponentially decays along the surrounding medium [8,9]. Let us call  $n_{eff}$  the effective index of the waveguide mode and  $n_{sample}$  the refractive index of the medium in the region where the so-called evanescent field decays; then the characteristic penetration depth (i.e. the distance,  $d$ , at which the evanescent field amplitude decreases by a factor of  $1/e$ ) is determined by Eq. (1) [1,10,11].

$$d = \frac{\lambda}{2\pi} \frac{1}{\sqrt{n_{eff}^2 - n_{sample}^2}} \quad (1)$$

From Eq. (1) and considering that  $n_{eff} > n_{sample}$ , it is clear that in the visible range the evanescent field of a waveguide provides a sensing region which is confined to a thickness  $< 200$  nm [6,12]. The evanescent-field approach has been used during the last

years for the development of a large variety of both label free and marked biosensors [13,14]. Among others, it has been reported the fabrication of glass [11], polymer [10,15], and semiconductor [16,17] planar waveguides for total internal reflection fluorescence (TIRF) microscopy. It is worth of note the commercially available "zeptosense" system [17] that by combining the evanescent-field and fluorescent methods can reach a detection limit of 0.8 zeptomoles for a spot diameter of 150  $\mu\text{m}$  (i.e. a surface concentration of  $10^{-18}$  mol/cm<sup>2</sup>), and a wide dynamical range. Other commercially available biosensors are based on label-free methods where the transduction process involves the modification of the effective refractive index induced by the immobilization of the analyte onto the core. Some examples of these system are the resonant-wavelength-grating based biosensor "OWLS<sup>TM</sup> 210" [18] (sensitivity  $\sim 1$  ng/cm<sup>2</sup>) and the single beam grating coupled interferometer developed by Creoptix [19] (surface sensitivity  $\sim 0.01$  ng/cm<sup>2</sup>). Note that a surface sensitivity of 1 ng/cm<sup>2</sup> entails a surface concentration of  $\sim 10^{-12}$  mol/cm<sup>2</sup> for a molecular weight of 397.8 Da corresponding to the fluorescent analyte here used. Some excellent reviews [13,14] provide comparative information about these and other optical biosensors. They show the higher potential sensitivity of the fluorescent and evanescent-field combined solutions in comparison with the label-free systems. However most of the TIRF biosensors are based on planar waveguides in which the excitation beam is coupled into the structure by prisms or by objective lens. Therefore, in case of multichannel biosensors the fluorescent signal is excited at the same wavelength [17], which limits the choice of the fluorophore probes. In the present work, we prove the concept of an evanescent-wave biosensors based on silicon oxynitride channel waveguides. This design allows for the development of compact multichannel chips where each emission signal might be excited at different wavelengths. The structures are produced by CMOS fabrication

techniques that enable the mass scale production of inexpensive disposable photonic layers. As another novelty, during the fabrication process the topmost layer of the photonic layer is adapted for the immobilization of biomolecules containing free amino ( $\text{NH}_2$ ) groups by a further wet chemical process.

Photonic biosensors based on Si compatible materials offer the advantage of exploiting the well-established CMOS micro-fabrication technologies for the development of densely packed multichannel arrays within a single chip. In addition, these techniques enable the development of monolithic systems in which the optical transducer is integrated together with the optoelectronic components of the sensor chip. Within CMOS compatible materials, silicon oxynitride (SiON) has proved to be a good candidate for the development of both marked and label free biosensors, including Mach-Zehnder interferometers, Fabry-Perot and disk resonators, as well as absorption based biosensors [20-23]. One of the main characteristics of this material lies in the flexibility to adjust the refractive index within a wide range as a function of the nitride content, from 1.45 ( $\text{SiO}_2$ ) to 2.00 ( $\text{Si}_3\text{N}_4$ ) [24,25]. Furthermore, SiON/ $\text{SiO}_2$  waveguides are particularly appealing for dye labeled biosensors, thanks to their low optical losses in the UV-visible region. For instance propagation losses as low as 1 dB/cm at 633 nm were reported for waveguides grown by plasma enhanced chemical vapor deposition (PECVD) [23,26].

The present paper reports about an evanescent-wave and fluorescent based optical transducer consisting of a SiON/ $\text{SiO}_2$  channel waveguide where a reactor well has been formed for the delivery of biological sample solutions. This system has been conceived as the photonic layer of a fully integrated chip biosensor incorporating the microfluidic and optoelectronic systems required for the detection process. As a main novelty the  $\text{SiO}_2$  cladding was removed along the sensing area while preserving a thinned SiON

core. According to our FDTD simulation, the optical mode still propagates through the thinned waveguide core while its evanescent tail spills out into the bioreactor region [27]. These simulations also indicate that the illumination of the sensing volume is homogenous and confined to a few tens of nm from the surface of the channel waveguide. In agreement with Eq. (1) the thickness of the sensing volume can be easily adjusted to different analyte dimensions either by controlling the refractive index of the solution filling the bioreactor well [27] or by changing the excitation beam wavelength.

In our previous work the fluorescence emission collected by the SION core was theoretically analyzed. In contrast, in this work we experimentally test the performance of the structure when collecting the fluorescence emission from the top of the bioreactor well. We use this vertical detection configuration in order to reproduce the design of the whole biosensor device where the photonic layer will be implemented. In this final device the photonic structure is interfaced with an *ad hoc* SPAD photodiodes matrix, which can be much more easily aligned on the top of the bioreactor. The present experimental work deals with the surface detection of dye molecules immobilized on the bioreactor bottom surface. This requires to adapt the composition of the bottom surface of the bioreactor for the immobilization of the fluorescent analyte. For these experiments we used as fluorescent analyte 5-(Aminomethyl)fluorescein -AMF- dye molecules: a green emitting xanthene derivative, which is commonly used as immunodiagnostic fluorescent probe [28].

## **Device description and detection set-up**

The overall layout of the prototype device is presented in Fig. 1(a) (more details in Ref. [27]). Main components of the optical layer are a set of channel waveguides and the micrometric reactor site for the analyte immobilization. For the detection

experiments a laser beam is butt-coupled into the input waveguide and transmitted toward the bioreactor where the fluorescent emission is excited. The structure also includes a Y splitter before the bioreactor. Thus, the reference branch allows monitoring the stability of the excitation beam and the reproducibility of the alignment independently of the absorption losses caused by the bioreactor content.

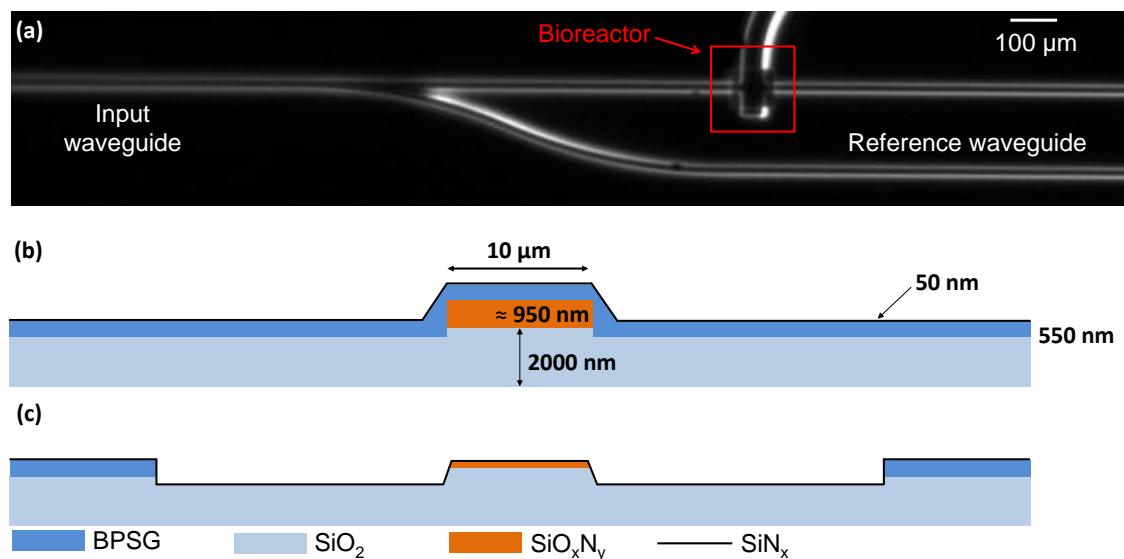


Fig. 1. Device description. (a) Optical image of the top view of the photonic layer. (b, c) Schematic cross-sections of the waveguide structure before (b) and at the bioreactor well (c). Note that in pictures (b) and (c) there is a scale factor of 2 between the vertical and horizontal dimensions.

The structures were fabricated in a standard silicon fabrication line by plasma enhanced chemical vapor (PECVD) and low pressure chemical vapor (LPCVD) deposition processes in combination with: 1100 °C annealing treatments to remove light-absorbing hydrogen bonds; and optical lithography for (pattern definition) and dry reactive ion etching (RIE) for the pattern transfer process. Figure 1 shows a schematic representation of the transversal cross section of the waveguide before and at the bioreactor well. As illustrated in Fig. 1(b) the waveguide structure consists of a 2- $\mu$ m-

thick SiO<sub>2</sub> buffer layer ( $n = 1.45$ ) and a 1- $\mu\text{m}$ -thick SiO<sub>x</sub>N<sub>y</sub> core layer ( $n = 1.85$ ) both deposited by PECVD; a  $\sim 0.5$ - $\mu\text{m}$ -thick borophosphosilicate glass (BPSG) layer ( $n = 1.45$ ) grown by LPCVD in order to optimize the surface planarity after RIE plays the role of the top cladding [29]. The waveguide was 10  $\mu\text{m}$  wide to better match the dimension of the bioreactor. Fabrication of bioreactor well (Fig. 1(c)) was also carried out by lithography/RIE. In this process the etching time was adjusted to completely remove the BPSG top cladding, as well as, to thin the core of the waveguide section that crosses the bioreactor. This is done in order to decrease the confinement of the propagating modes and therefore to increase the interaction between the evanescent field and the bioreactor content. Finally, the whole system was coated with a thin SiN<sub>x</sub> film (50 nm of thickness) intended to accommodate the surface chemical composition of the structure [for the immobilization of amino containing biomolecules](#) by the chemical process described below; but without disturbing the optical properties of the photonic layer. It is important to remark that both, the design of the channel waveguide and the fabrication protocol, have been optimized for the production of low losses waveguides in the visible range where organic dyes are excited and emit, with propagation losses below 3 dB/cm at  $\lambda = 473$  nm. To illustrate this point, Fig. 2(b) shows the propagation of a 473-nm excitation beam up to the micro-bioreactor as well as the beam transmitted after the micro-bioreactor. The bioreactor and the waveguide dimensions are also dictated by the requirement of a sensing area large enough to be potentially functionalized by a spotter with the trapping agent (i.e., to deliver the recognition element onto the active sensor surface). Therefore a 50x50  $\mu\text{m}^2$  bioreactor site was selected, and a waveguide width of 10  $\mu\text{m}$  was chosen to interact with a representative area of the bottom surface of the bioreactor.



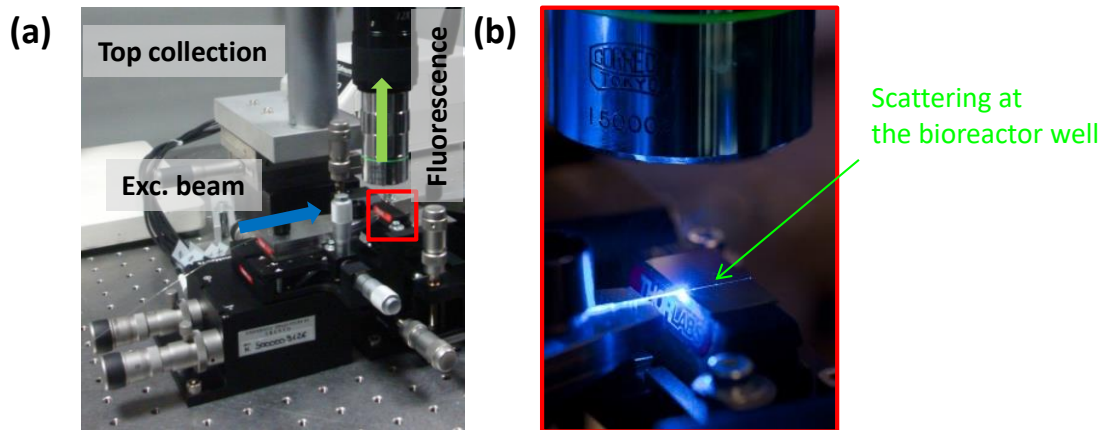


Fig. 2. (a) Photograph of the experimental set-up used for the detection test. The photonic chip is located on the sample holder within the red square. (b) Enlarged view of the photonic chip when a 473-nm blue laser beam is propagating through the structure. Note that the light signal is propagating all over the chip from the input facet to the output facet. The bright point at midway is the location of the reactor and the spot is due to the scattering of the light at this location.

For the detection experiments a homemade modular experimental set-up was used (Fig. 2(a)). The excitation section consists of a DPSS laser source at 473 nm (CIEL from Laser Quantum) coupled to a tapered optical fiber which is mounted on a piezoelectric micropositioning system for the alignment process. The optical transducer herein analyzed has been devised for its further implementation into a portable biosensor device in which the fluorescence signal is detected by a SPAD photodetector array installed over the photonic layer. In order to emulate this architecture, in our experimental system the fluorescence emission is collected from the top of the structure. The detection system consists of an objective lens (20X) coupled with an ultra-zoom (12X maximum magnification) to achieve a field of view of the same order of magnitude of the bioreactor area. The collected emission is coupled by a set of lens and optical fibers into a spectrometer (SOPRA DMS2) interfaced with a cooled photomultiplier tube.

## Results.

To check the suitability of the photonic layer for the fluorescent detection of fluorescent analytes two different kinds of studies have been carried out by employing AMF as fluorescent marker. In the first series of experiments volumetric sensing has been performed. In this case, the bioreactor was filled with different AMF-water solutions; therefore the detection of the dye molecules in water is analyzed. Figure 3 shows the various emission spectra acquired for different dye concentrations. Emission is here excited by the laser beam propagating in the waveguide and collected from the top of the structure. As shown in Fig. 3, the emission maxima are located in the 500-550 nm spectral region which corresponds to the emission range of AMF molecules in water solution. This confirms the suitable excitation of the fluorescent dye by the laser beam transmitted through the bioreactor. For a high dye concentration of  $10^{-3}$  M the green emission from the dye solution is strong enough to be detected by visual inspection through the microscope; whereas it progressively decreases with the dye concentration. No linear relationship between the dye concentration and the emission intensity was observed in our experiments. This result may be due to two different factors: first reabsorption of the fluorescent emission as a consequence of the overlapping of the emission and absorption bands and due to the localized excitation of the emission on the bottom of the reactor. Such a behavior is typically observed for high concentrations of organic dyes with a short Stokes shift, which is the case for AMF. The second factor is the formation of aggregated species with a lower quantum yield that leads to the reduction of the emission efficiency as the dye concentration increases. This is a common effect in xanthene derivatives molecules that is accompanied by a red shift of the emission band [30,31]. In fact, this phenomenon also explains the red-shift of the emission maximum observed in Fig. 3 as the dye concentration increases. It is worth of

note that the minimum concentration that we were able to detect was  $10^{-8}$  M (see inset in Fig. 3), a value which is close to the limit of detection of other photonic biosensors [32].

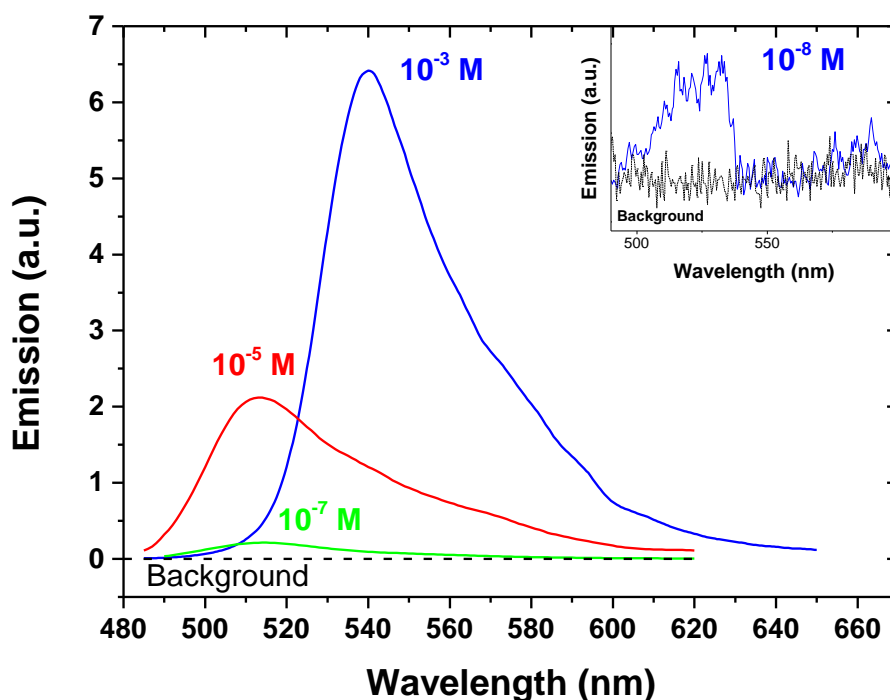


Fig. 3. Fluorescence spectra acquired for AMF-water solutions delivered in the bioreactor. The insert shows the emission for a  $10^{-8}$  M solution. The background line is measured with an empty bioreactor.

The second class of experiments was aimed at the surface sensing. Point of care and biosensing applications demand for a selective response towards the target molecule. This can be addressed by functionalizing the optical transducer with a biological layer for the specific recognition of the target analyte. Binding of biological molecules (which should form the recognition layer) on an inorganic surface requires an organic interlayer bearing reactive groups able to immobilize the desired bioreceptor. We set-up a simple

functionalization protocol to introduce an organic interface onto the microwells which exposes carboxylic (COOH) groups able to react with the amino group and form an amide bond. These groups can be used to immobilize biomolecules containing free amino groups. To test the performances of the functionalized surface integrated in the sensor chip, we anchored a fluorescent marker bearing an amino group (AMF) to the functionalized sensor surface.

Wet chemical functionalization of the thin SiN<sub>x</sub> final layer of the photonic structure was carried out by the process summarized in Fig. 4. Before functionalization the samples were cleaned by sonication in trichloroethylene, acetone and 2-propanol. Afterwards they were immersed in a 2% HF solution (1 min) to remove the native oxide, rinsed with water and dried under a gentle nitrogen flux. Thereupon, in order to introduce the carboxylic groups, the samples were immersed into a 0.08 M solution of Br-dodecanoic acid (Br-(CH<sub>2</sub>)<sub>11</sub>-COOH) in toluene and kept under reflux (110°C) in argon atmosphere for 120 min [33]. The samples were then rinsed by sonication in dichloromethane, acetonitrile, water and methanol and dried with nitrogen. Carboxyl moieties immobilized inside the microreactors were then marked using AMF. First the carboxylic groups were activated by dipping the photonic chips into a solution of 75 mM N-(3-dimethylaminopropyl)-N'-ethyl-carbodiimide hydrochloride (EDC) and 15 mM N-hydroxysulfosuccinimide sodium salt (NHSS) for 30 min [34]. Then the samples were rinsed with water, dried with nitrogen and the microwells were immediately spotted with a 100 μM AMF solution. The dye was dissolved into DMSO: 0.1 M phosphate buffer, pH 8 (1:9), which was proved to provide a good reaction medium. For the spotting process a BioOdyssey Calligrapher MiniArrayer, BIO-RAD, with a 100μm capillary tip was used. After spotting, the samples were stored in the dark for an incubation time of 120 min. Afterwards, the samples were thoroughly rinsed in the

DMSO-phosphate buffer solution and in water in order to remove those dye molecules that are not chemically bond to the bioreactor surface. Finally they were dried under a nitrogen flow. The same functionalization process was carried out on a set of reference silicon nitride layers that were analyzed in a commercial spectrofluorometer. These analyses revealed that after the final cleaning process a surface concentration  $10^{-11}$  mol/cm<sup>2</sup> of fluorescent AMF molecules remains immobilized on the SiN<sub>x</sub> layer. The good performance of the spotting process was also tested by fluorescence microscopy (see Fig. 6(a) presented below).

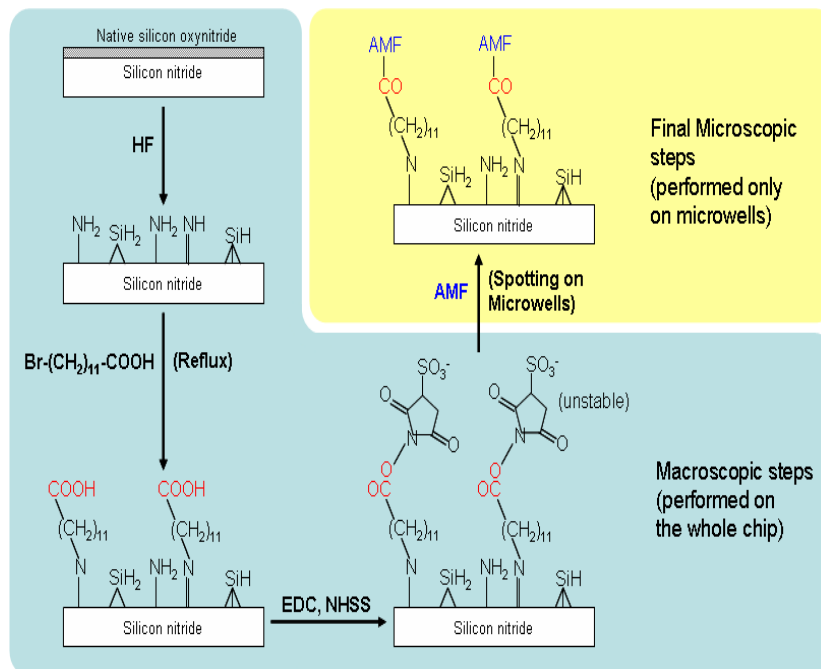


Fig. 4. Scheme of the chemical reactions used for the immobilization of the AMF molecules on the bioreactor.

As a representative example, Fig. 5 shows the emission spectrum recorded for a functionalized bioreactor with a dye surface concentration of  $10^{-11}$  mol/cm<sup>2</sup>. This spectrum depicts a weak broad emission band extending from 500 – 550 nm, which is the emission spectral region of AMF. This result proves the excitation of the immobilized AMF molecules by means of the evanescent field of the waveguide, as

well as the capability of the system to detect low surface concentrations of this dye ( $10^{-11}$  mol/cm<sup>2</sup>). Indeed considering the bioreactor area (2500  $\mu\text{m}^2$ ) this surface concentration entails an amount of  $10^{-16}$  moles of AMF in the bioreactor bottom surface. Nevertheless, this surface concentration is higher than the sensitivity of other biosensors described in the introduction. At this point it is important to stress that this is not an optimized device, and that this study just aims to experimentally demonstrate the concept of CMOS-fabricated SiON channel waveguides for the surface detection of immobilized fluorescent molecules. Some issues to be solved are related to the photobleaching of the dye and the anisotropy of the fluorescence emission. In our preliminary experiments, we noticed that the AMF molecules undergo a fast photodegradation. The AFM bleaching was demonstrated by analyzing some reference samples by fluorescence microscopy, before and after exposing them to the laser beam (see later). For this reason we suppose that in the absence of bleaching the signal shown in Figure 5 could be much more intense. In fact the sensor detection test in Fig. 5 requires the alignment of the optical set-up, a process during which the immobilized dye molecules is exposed to the excitation laser beam for at least two min. In addition, it is also important to take into account that the Fermi golden rule states that the spontaneous radiation rate is affected by the photon mode density which in turn is determined by the dielectric environment. Thus, as it was experimentally reported and theoretically analyzed [35,36], the emission from the dye molecules at the waveguide core interface is not isotropic; and most of the energy is radiated toward the high refractive index material (i.e. the waveguide core). Nevertheless our experimental results prove the suitability of the photonic layer to detect low surface concentration of a fluorescent analyte even under such adverse conditions (i.e. dye photobleaching and detection from the top of the structure).

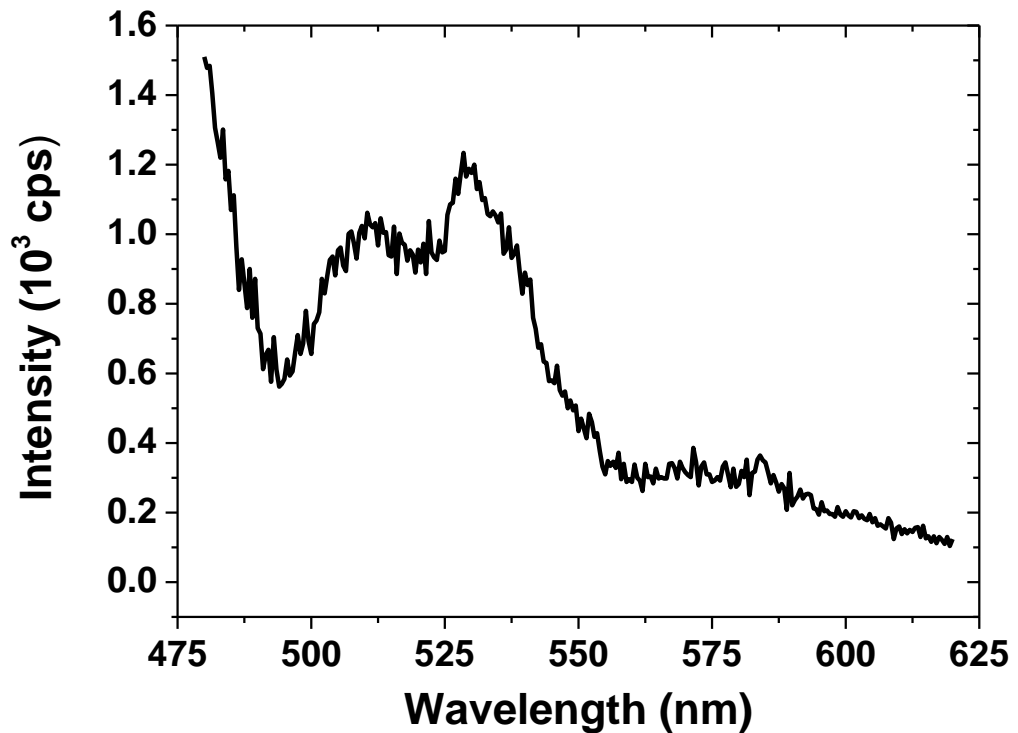


Fig. 5. Emission spectrum recorded for a functionalized bioreactor with an AMF surface concentration of  $10^{-11}$  mol/cm<sup>2</sup>.

Further proofs of the interaction between the evanescent field and the trapped dye molecules are provided in Fig. 6. This figure shows in (a) the fluorescence image recorded on the bioreactor just after the functionalization and (b) the fluorescence image of the same bioreactor after the surface sensing experiment. In Fig. 6(b) it is apparent the photobleaching of the AMF molecules caused by the propagation of the laser in the waveguide. Photodegradation affects only those AMF molecules immobilized on the surface of the waveguide. This evidences that the excitation of the dye is due to the evanescent field of the propagating mode. Hence, the excitation is very localized (note that the other AMF molecules preserve their luminescence activity) in agreement with our previous theoretical FDTD simulations [26]. This opens the possibility of using the functionalized structures for the specific detection of a target molecule without the need

of the final cleaning procedure, even when analyzing complex samples containing different **fluorescent** biomolecules, as discussed in the introduction.

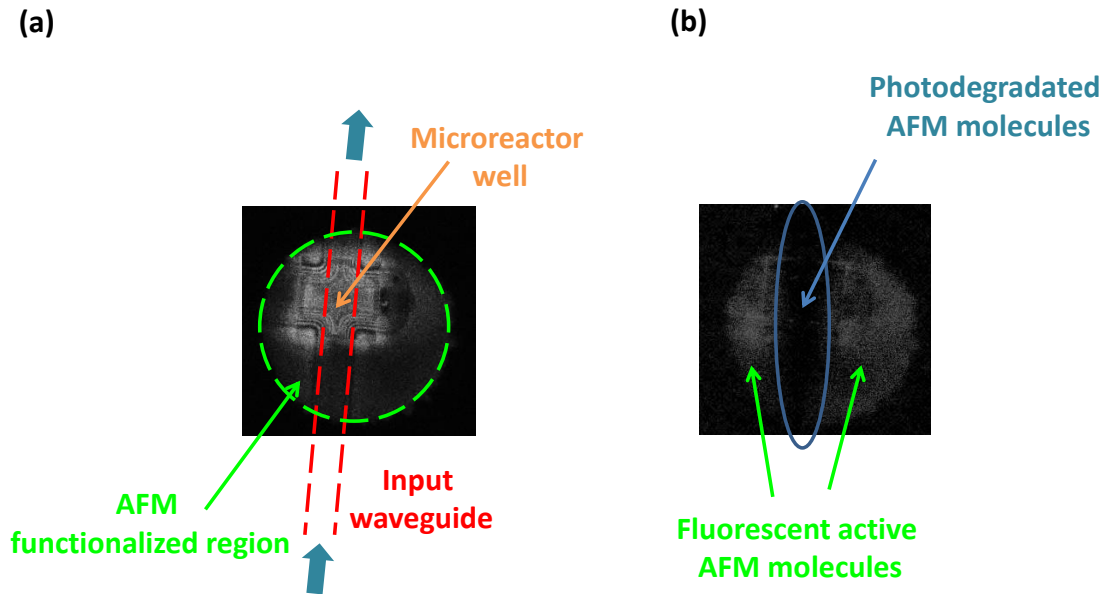


Fig. 6. Fluorescence microscopy image of a micro-bioreactor (a) after the functionalization process and (b) after a prolonged detection experiment.

### Conclusions and summary.

A SiON channel waveguide based optical transducer has been developed and tested. This simple photonic layer has been conceived for its implementation in a modular-stack lab-on-chip biosensor. The working concept is based on the **fluorescent** detection of the fluorophore markers excited by means of the evanescent field propagating through the waveguide. In this way, a very localized excitation of the fluorescence is possible. In order to selectively detect a given biomolecule, the structure can be functionalized with a biorecognition layer for the specific immobilization of the target



molecules. As a proof of concept the photonic layer has been successfully applied in the fluorescent detection of AMF molecules bound to the bottom of a bioreactor, for a low dye surface concentration of  $10^{-11}$  mol/cm<sup>2</sup>. In these experiments the photobleaching pattern observed after illumination confirms that the dye excitation is mainly mediated by the evanescent field of the optical modes propagating in the SiON waveguide. In addition, the penetration depth of the evanescent-wave (i.e. the thickness of the interrogation volume) can be easily adjusted as a function of the refractive index of the bioreactor content (cf. Eq. (1)). Thus, by filling the reactor well with the suitable solvent the system might allow for the detection of larger analytes [37]. These characteristics together with the possibilities of the employed fabrication techniques (CMOS fabrication techniques) allow to extend the design to the development of a single-system sensors array with multianalyte capabilities, by functionalizing each single sensing structure with a specific biorecognition layer.

## Acknowledgments

This work was supported by PAT in the framework of the FU-PAT NAOMI project.

## References.

- [1] Seitz P, "Optical Biochips," in *Biophotonics*, L. Pavesi, and P. Fauchet, Eds. (Springer-Verlag Berlin Heidelberg, 2008).
- [2] Janasek D, Franzke J, and Manz A, 2006 *Nature* **442**, 374.
- [3] Kostov Y, and Rao G, 2000 *Rev. Sci. Instrum.* **71**, 4361.
- [4] Templin M F, Stoll D, Schwenk J M, Pötz O, Kramer S, and Joos T O, 2003 *Proteomics* **3**, 2155.
- [5] Seong S-Y, and Choi C-Y, 2003 *Proteomics* **3**, 2176.
- [6] Passaro V, Dell'Olio F, Casamassima B, and De Leonardis F, 2007 *Sensors* **7**, 508.
- [7] Patel P N, Mishra V, and Mandloi A S, 2012 *Journal of Engineering Research and Studies* **1**, 15.
- [8] Bahaa E. A. Saleh, and Malvin Carl Teich, *Fundamentals of Photonics* (John Wiley & Sons, Inc., New York, 1991).
- [9] Hunsperger R G, *Integrated Optics: Theory and Technology* (Springer Science & Business Media, New York, 2009).
- [10] Agnarsson B, Ingthorsson S, Gudjonsson T, and Leosson K, 2009 *Opt. Express* **17**, 5075.

- [11] Ramachandran S, Cohen D A, Quist A P, and Lal R, 2013 *Sci. Rep.* **3**.
- [12] Kunz R, and Cottier K, 2006 *Anal. Bioanal. Chem.* **384**, 180.
- [13] Mukundan H, Anderson A, Grace W K, Grace K, Hartman N, Martinez J, and Swanson B, 2009 *Sensors* **9**, 5783.
- [14] Rich R L, and Myszka D G, 2005 *Journal of Molecular Recognition* **18**, 1.
- [15] Agnarsson B, Jonsdottir A B, Arnfinnsdottir N B, and Leosson K, 2011 *Opt. Express* **19**, 22929.
- [16] Duveneck G L, Abel A P, Bopp M A, Kresbach G M, and Ehrat M, 2002 *Anal. Chim. Acta* **469**, 49.
- [17] Pawlak M, Schick E, Bopp M A, Schneider M J, Oroszlan P, and Ehrat M, 2002 *Proteomics* **2**, 383.
- [18] [www.owls-sensors.com](http://www.owls-sensors.com)
- [19] Patko D, Cottier K, Hamori A, and Horvath R, 2012 *Opt. Express* **20**, 23162.
- [20] Lambeck P V, 2006 *Meas. Sci. Technol.* **17**, R93.
- [21] Nunes P S, Mortensen N A, Kutter J P, and Mogensen K B, 2008 *Opt. Lett.* **33**, 1623.
- [22] Klunder D, Elders J, Burger G-J, Amersfoort M, Krioukov E, Otto C, Hoekstra H, and Driessen A, *Proc. SPIE 5269, Chemical and Biological Point Sensors for Homeland Defense*, (2004) doi: 10.1117/12.515862.
- [23] Mogensen K B, Friis P, Hübner J, Petersen N, Jørgensen A M, Telleman P, and Kutter J P, 2001 *Opt. Lett.* **26**, 716.
- [24] Lianghong Y, Ming L, Leszek W, Weiwei S, Jun T, Yicheng L, and Wei J, 2012 *Journal of Optics* **14**, 085501.
- [25] De Ridder R M, Warhoff K, Driessen A, Lambeck P V, and Albers H, 1998 *Selected Topics in Quantum Electronics, IEEE Journal of* **4**, 930.
- [26] Han B, *et al.*, *Proc. SPIE 8069, Integrated Photonics: Materials, Devices, and Applications, 80690K*, (2011) doi: 10.1117/12.886820.
- [27] Rigo E, Aparicio F J, Vanacharla M R, Larcheri S, Guider R, Han B, Pucker G, and Pavesi L, 2013 *Appl. Phys. B*, 1.
- [28] Shipchandler M T, Fino J R, Klein L D, and Kirkemo C L, 1987 *Anal. Biochem.* **162**, 89.
- [29] Ghulinyan M, Guider R, Pucker G, and Pavesi L, 2011 *Photonics Technology Letters, IEEE* **23**, 1166.
- [30] López Arbeloa F, Martínez Martínez V, Arbeloa T, and López Arbeloa I, 2007 *Journal of Photochemistry and Photobiology C: Photochemistry Reviews* **8**, 85.
- [31] Aparicio F J, Borrás A, Blaszczyk-Lezak I, Gröning P, Álvarez-Herrero A, Fernández-Rodríguez M, González-Elipé A R, and Barranco A, 2009 *Plasma Processes and Polymers* **6**, 17.
- [32] Cleary A, Glidle A, Laybourn P J R, Garcia-Blanco S, Pellegrini S, Helfter C, Buller G S, Aitchison J S, and Cooper J M, 2007 *Appl. Phys. Lett.* **91**, 071123.
- [33] Cattaruzza F, Cricenti A, Flamini A, Girasole M, Longo G, Mezzi A, and Prospero T, 2004 *J. Mater. Chem.* **14**, 1461.
- [34] Wang J, Profitt J A, Puglia M J, and Suni I I, 2006 *Anal. Chem.* **78**, 1769.
- [35] Baldini F, Carloni A, Giannetti A, Porro G, and Trono C, 2008 *Anal. Bioanal. Chem.* **391**, 1837.
- [36] Burke C, Stránik O, McEvoy H, and MacCraith B, "Planar Optical Sensors and Evanescent Wave Effects," in *Optical Chemical Sensors*, F. Baldini, A. N. Chester, J. Homola, and S. Martellucci, Eds. (Springer Netherlands, 2006).
- [37] Horvath R, Cottier K, Pedersen H C, and Ramsden J J, 2008 *Biosens. Bioelectron.* **24**, 799.